



VASO-OCCLUSIVE DEVICES WITH IN-SITU STIFFENING
Stephen C. Porter
10/695,151

1/6

FIG. 1

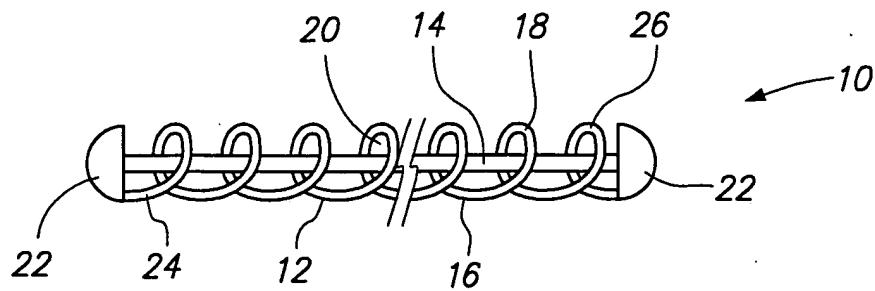


FIG. 2


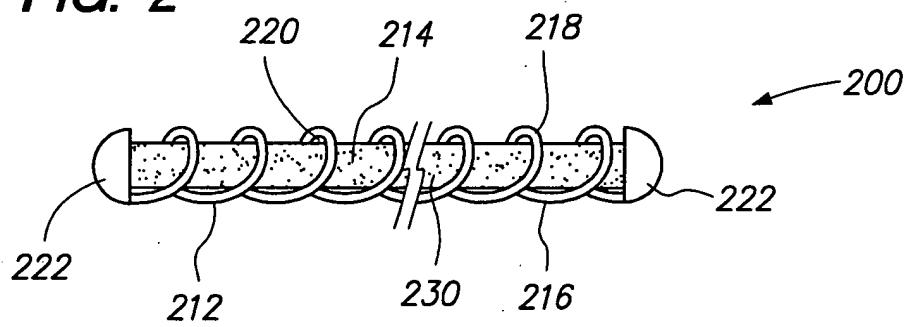


FIG. 3

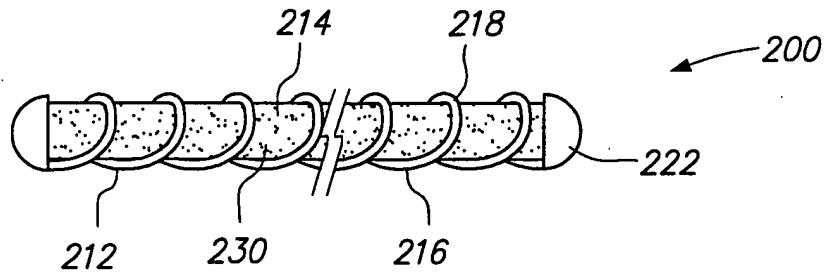

2/6

FIG. 4

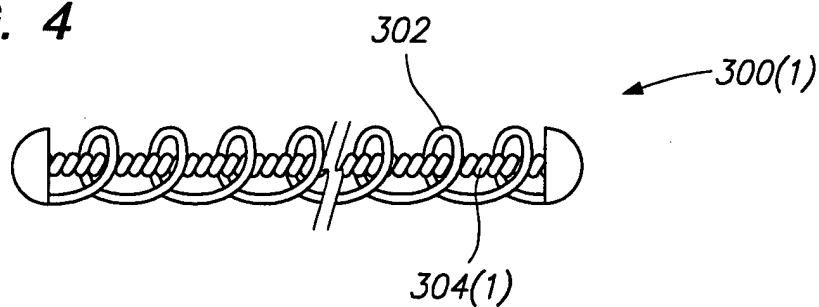


FIG. 5


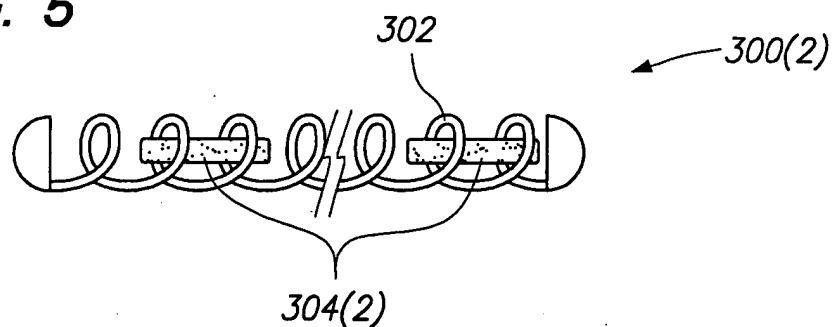


FIG. 6

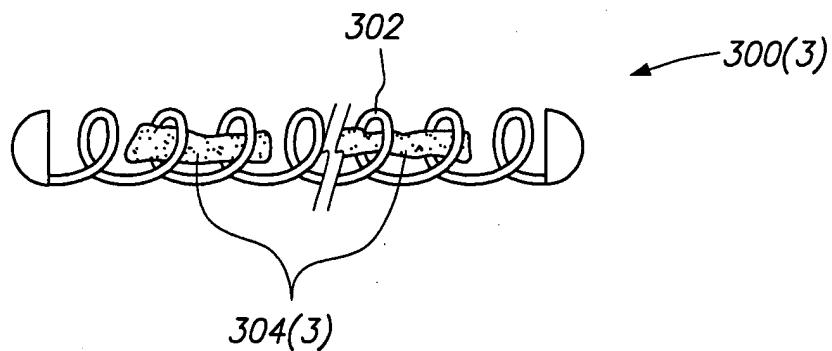

3/6

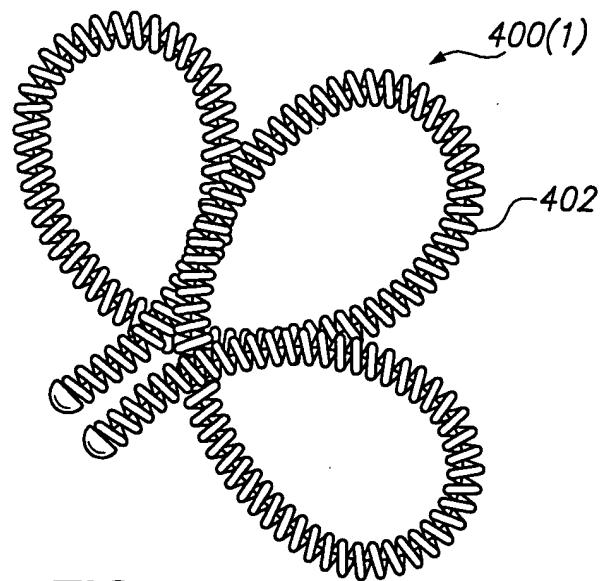


FIG. 7

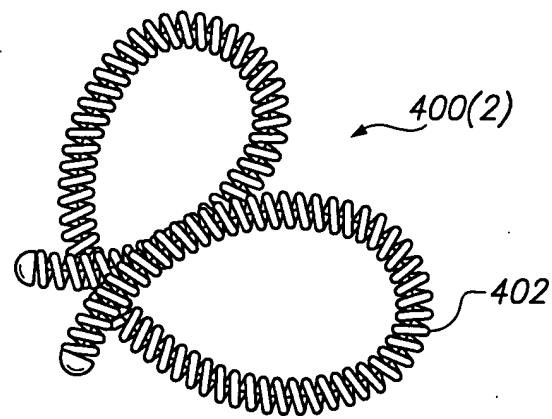


FIG. 8

4/6

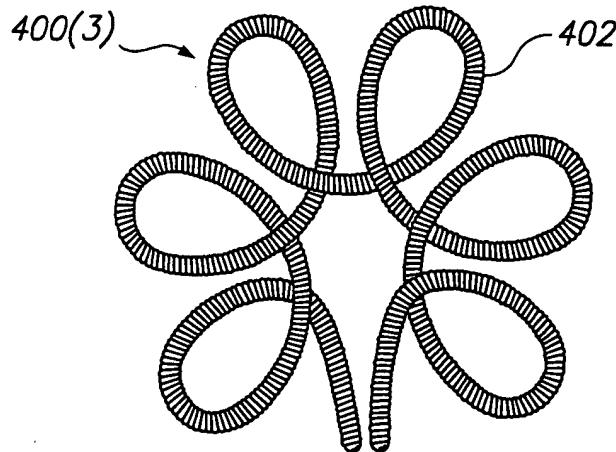


FIG. 9

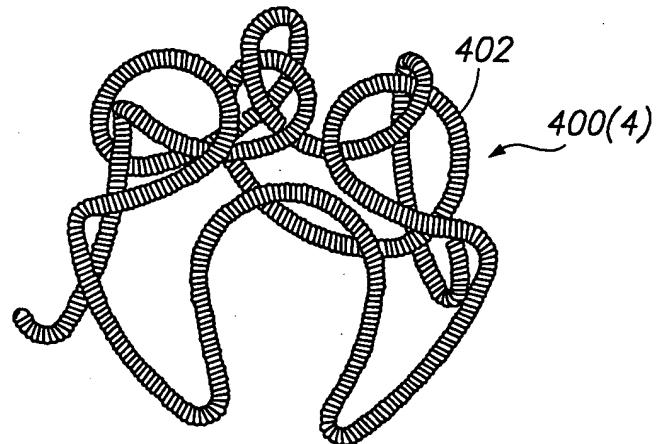


FIG. 10

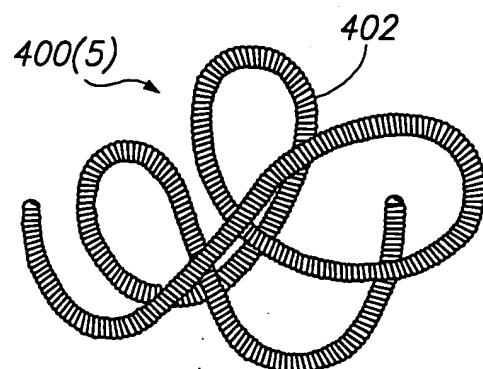


FIG. 11

MULTI-ZONE BIPOLAR ABLATION PROBE ASSEMBLY
Kimbolt Young, et al
10/684,086

5/6

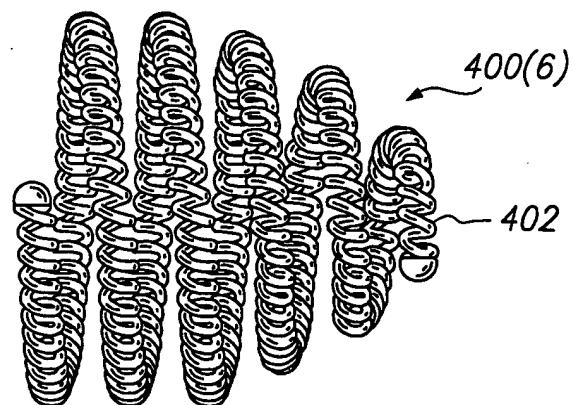


FIG. 12

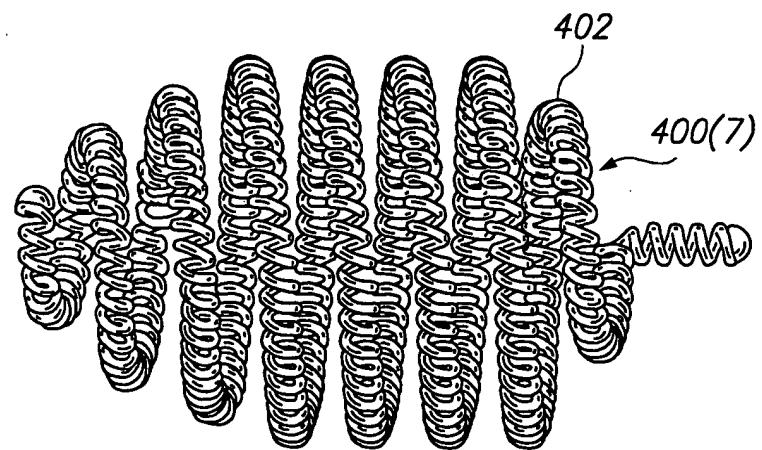


FIG. 13

6/6

FIG. 14

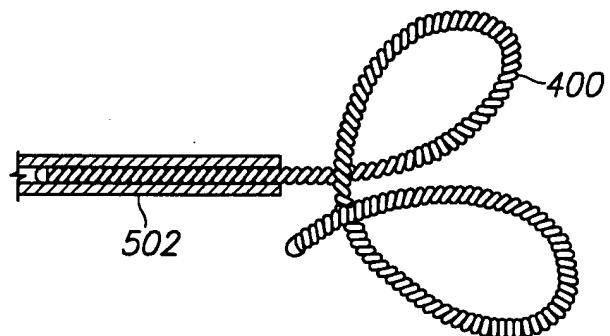
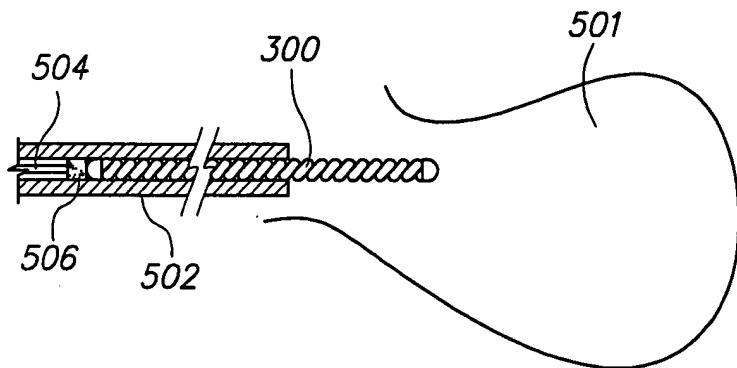


FIG. 15

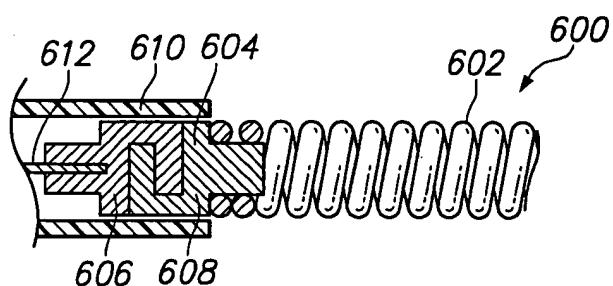


FIG. 16

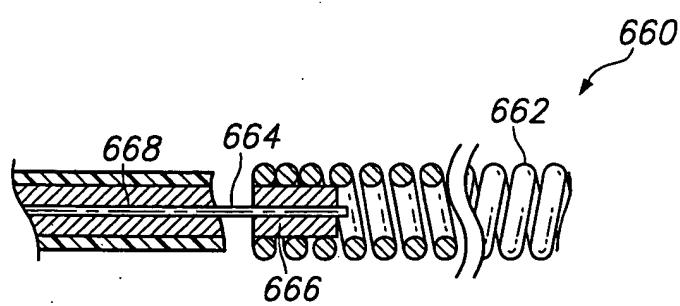


FIG. 17